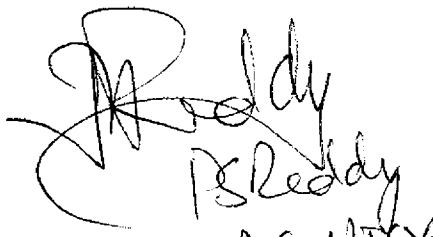


TECHNICAL SPECIFICATION FOR PORTABLE CONDUCTIVITY METER

#	Specification	Range/Requirement
1	Measurement Type	Using conductivity electrode with BNC end cable
2	Range	1 μ S/cm to 200 mS/cm
3	Accuracy	± 1 % F.S
4	Resolution	0.2 μ S/cm
5	Operating temperature	0-45 °C
6	Temperature compensation	Automatic or manual
7	Calibration	1 point calibration/Automatic with buffer solution for min 2 calibration
8	Power	Battery operated/with suitable AC adaptor for 220V/50Hz
9	Carrying case	Hard carrying case
10	Display	Backlite LCD
11	Documents	O & M Manual 2 copies and 1 CD
12	Guarantee	18 months from date of delivery
13	Calibration Certificate	Calibration certificate for one year
14	Catalogue	Along with Technical Bid detailed manual with specification for the quoted model to be supplied. Catalogue should be original.


R. S. Reddy
AGM/ISY